


LITERATURE REVIEW

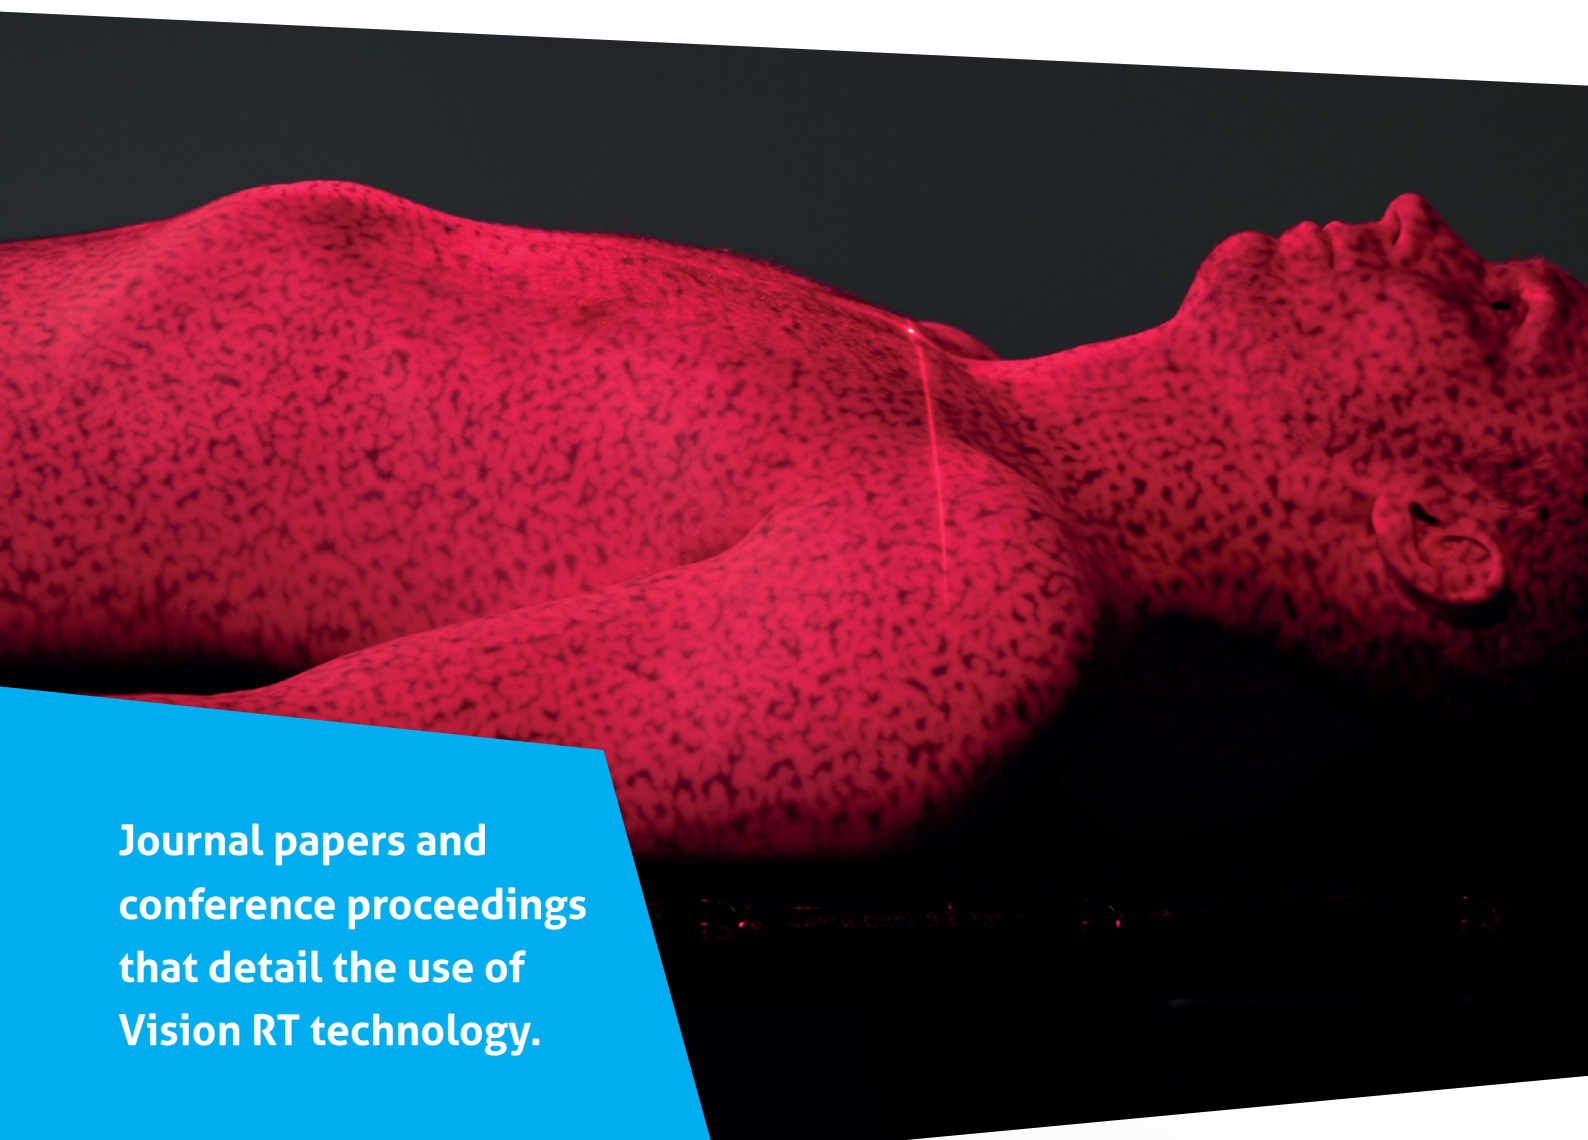

**Journal papers and
conference proceedings
that detail the use of
Vision RT technology.**

visionrt

Defining the Standard of Care in
SURFACE GUIDED RADIATION THERAPY

JOURNAL PAPERS AND CONFERENCE PROCEEDINGS THAT DETAIL THE USE OF VISION RT TECHNOLOGY.

Breast DIBH

Cervino, L. I., et al. (2009).

"Using surface imaging and visual coaching to improve the reproducibility and stability of deep-inspiration breath hold for left-breast-cancer radiotherapy."

[Phys Med Biol 54\(22\): 6853-6865.](#)

Cheung, Y., et al. (2015).

"SU-F-BRB-03: Quantifying Patient Motion During Deep-Inspiration Breath-Hold Using the ABC System with Simultaneous Surface Photogrammetry."

[Medical Physics 42\(6Part25\): 3530-3530.](#)

Flampouri, S., et al. (2008).

"Position Verification of Breast Treatment with Breath-Hold Technique Using 3D-Surface and Fluoroscopic Imaging."

[Medical Physics 35\(6\): 2713-2713.](#)

Gierga, D. P., et al. (2012).

"A voluntary breath-hold treatment technique for the left breast with unfavorable cardiac anatomy using surface imaging."

[Int J Radiat Oncol Biol Phys 84\(5\): e663-668.](#)

Lyatskaya, Y., et al. (2011).

"Validation of Align RT System for Breast Radiation Therapy with Deep Inspiration Breath Hold (DIBH) Technique."

[Med Phys 38.](#)

Rochet, N., et al. (2015).

"Deep inspiration breath-hold technique in left-sided breast cancer radiation therapy: Evaluating cardiac contact distance as a predictor of cardiac exposure for patient selection."

[Pract Radiat Oncol 5\(3\): e127-134.](#)

Rong, Y., et al. (2014).

"Improving intra-fractional target position accuracy using a 3D surface surrogate for left breast irradiation using the respiratory-gated deep-inspiration breath-hold technique."

[PLoS One 9\(5\): e97933.](#)

Tang, X., et al. (2015).

"Dosimetric effect due to the motion during deep inspiration breath hold for left-sided breast cancer radiotherapy."

[J Appl Clin Med Phys 16\(4\): 91-99.](#)

Tang, X., et al. (2014).

"Clinical experience with 3-dimensional surface matching-based deep inspiration breath hold for left-sided breast cancer radiation therapy."

[Pract Radiat Oncol 4\(3\): e151-158.](#)

Tanguturi, S. K., et al. (2015).

"Prospective assessment of deep inspiration breath-hold using 3-dimensional surface tracking for irradiation of left-sided breast cancer."

[Pract Radiat Oncol 5\(6\): 358-365.](#)

Zagar, T. M., et al. (2017).

"Utility of Deep Inspiration Breath Hold for Left-Sided Breast Radiation Therapy in Preventing Early Cardiac Perfusion Defects: A Prospective Study."

[Int J Radiat Oncol Biol Phys 97\(5\): 903-909.](#)

Breast FB

Bert, C., et al. (2006).

"Clinical experience with a 3D surface patient setup system for alignment of partial-breast irradiation patients."

[Int J Radiat Oncol Biol Phys 64\(4\): 1265-1274.](#)

Chang, A. J., et al. (2012).

"Video surface image guidance for external beam partial breast irradiation."

[Pract Radiat Oncol 2\(2\): 97-105.](#)

Deantonio, L., et al. (2011).

"Detection of setup uncertainties with 3D surface registration system for conformal radiotherapy of breast cancer."

[Rep Pract Oncol Radiother 16\(3\): 77-81.](#)

Gierga, D. P., et al. (2008).

"Comparison of target registration errors for multiple image-guided techniques in accelerated partial breast irradiation."

[Int J Radiat Oncol Biol Phys 70\(4\): 1239-1246.](#)

Herron, E., et al. (2018).

"Surface Guided Radiation Therapy as a Replacement for Patient Marks in Treatment of Breast Cancer."

[International Journal of Radiation Oncology • Biology • Physics 102\(3\): e492-e493.](#)

Magnelli, A., et al. (2012).

"Clinical Evaluation of a Three-Dimensional Optical Surface Based Imaging Device for Breast Treatment Setup."

[Med Phys 39.](#)

Miller, D. A., et al. (2008).

"Inter-fraction and Intra-fraction Breast Motion Localized using AlignRT for Early Breast Cancer."

[International Journal of Radiation Oncology • Biology • Physics 72\(1\): S189-S190.](#)

Padilla, L., et al. (2014).

"Assessment of interfractional variation of the breast surface following conventional patient positioning for whole-breast radiotherapy."

[J Appl Clin Med Phys 15\(5\): 4921.](#)

Riboldi, M., et al. (2007).

"Quantitative Assessment of Surface Deformation in Accelerated Partial Breast Irradiation."

[International Journal of Radiation Oncology • Biology • Physics 69\(3\): S669.](#)

Schoffel, P. J., et al. (2007).

"Accuracy of a commercial optical 3D surface imaging system for realignment of patients for radiotherapy of the thorax."

[Phys Med Biol 52\(13\): 3949-3963.](#)

Shah, A. P., et al. (2013).

"Clinical evaluation of interfractional variations for whole breast radiotherapy using 3-dimensional surface imaging."

[Pract Radiat Oncol 3\(1\): 16-25.](#)

Wiant, D., et al. (2012).

"SU-D-213CD-02: The Accuracy of AlignRT Guided Set-Up for Whole Breast and Chestwall Irradiation."

[Med Phys 39: 3617-3618.](#)

GateCT GateRT

Hughes, S., et al. (2009).

"Assessment of two novel ventilatory surrogates for use in the delivery of gated/tracked radiotherapy for non-small cell lung cancer."

[Radiother Oncol 91\(3\): 336-341.](#)

Noel, C., et al. (2008).

"A Surface-Based Respiratory Surrogate for 4D Imaging."

[Medical Physics 35\(6\): 2682-2682.](#)

Spadea, M. F., et al. (2010).

"Evaluation and commissioning of a surface based system for respiratory sensing in 4D CT."

[J Appl Clin Med Phys 12\(1\): 3288.](#)

Pediatric

Rwigema, J. M., et al. (2017).

"Palliative radiation therapy for superior vena cava syndrome in metastatic Wilms tumor using 10XFFF and 3D surface imaging to avoid anesthesia in a pediatric patient-a teaching case."

[Adv Radiat Oncol 2\(1\): 101-104.](#)

Sueyoshi, M., et al. (2018).

"Eliminating Daily Shifts, Tattoos, and Skin Marks: Streamlining Isocenter Localization With Treatment Plan Embedded Couch Values for External Beam Radiation Therapy."

[Practical Radiation Oncology.](#)

Patient Safety

Manger, R. P., et al. (2015).

"Failure mode and effects analysis and fault tree analysis of surface image guided cranial radiosurgery."

[Med Phys 42\(5\): 2449-2461.](#)

Wiant, D. B., et al. (2016).

"A novel method for radiotherapy patient identification using surface imaging."

[J Appl Clin Med Phys 17\(2\): 271-278.](#)

Pelvis

Apicella, G., et al. (2016).

"Three-dimensional surface imaging for detection of intra-fraction setup variations during radiotherapy of pelvic tumors."

[Radiol Med 121\(10\): 805-810.](#)

Proton

Batin, E., et al. (2016).

"Can surface imaging improve the patient setup for proton postmastectomy chest wall irradiation?"

[Pract Radiat Oncol 6\(6\): e235-e241.](#)

Mutter RW, et al. (2017).

Initial clinical experience of postmastectomy intensity modulated proton therapy in patients with breast expanders with metallic ports.

[Practical Radiation Oncology 2017:7\(4\):e243-e252.](#)

Sarcoma

Gierga, D. P., et al. (2014).

"Analysis of setup uncertainties for extremity sarcoma patients using surface imaging."

[Pract Radiat Oncol 4\(4\): 261-266.](#)

SBRT

Heinzerling, J. H., et al. (2017).

"Use of 3D Optical Surface Mapping for Quantification of Interfraction Set up Error and Intrafraction Motion during Stereotactic Body Radiation Therapy Treatments of the Lung and Abdomen."

[International Journal of Radiation Oncology • Biology • Physics 99\(2\): E670](#)

SRS

Baker, B., et al. (2013).

"Trigeminal Rhizotomy Performed with Modern Image-guided Linac: Case Report."

[Cureus 5\(9\): e139.](#)

Cervino, L. I., et al. (2012).

"Initial clinical experience with a frameless and maskless stereotactic radiosurgery treatment."

[Pract Radiat Oncol 2\(1\): 54-62.](#)

Cervino, L. I., et al. (2010).

"Frame-less and mask-less cranial stereotactic radiosurgery: a feasibility study."

[Phys Med Biol 55\(7\): 1863-1873.](#)

Chinsky, B., et al. (2016).

"Feasibility of Using a Commercially Available Surface Guided

Radiotherapy System with An Open-Face SRS Immobilization System."

[Medical Physics 43\(6\): 3611-3611.](#)

Covington EL, et al. (2019).

Optical surface guidance for submillimeter monitoring of patient position during frameless stereotactic radiotherapy.

[Journal of Applied Clinical Medical Physics 2019](#)

Lau, S. K., et al. (2017).

"Clinical efficacy and safety of surface imaging guided radiosurgery (SIG-RS) in the treatment of benign skull base tumors."

[J Neurooncol 132\(2\): 307-312.](#)

Lau, S. K., et al. (2015).

"Single-Isocenter Frameless Volumetric Modulated Arc Radiosurgery for Multiple Intracranial Metastases."

[Neurosurgery 77\(2\): 233-240: discussion. 240.](#)

Li, G., et al. (2015).

"Clinical experience with two frameless stereotactic radiosurgery (fSRS) systems using optical surface imaging for motion monitoring."

[J Appl Clin Med Phys 16\(4\): 149-162.](#)

Li, G., et al. (2011).

"Motion monitoring for cranial frameless stereotactic radiosurgery using video-based three-dimensional optical surface imaging."

[Med Phys 38\(7\): 3981-3994.](#)

Li, G., et al. (2011).

"Optical Surface Imaging for Online Rotation Correction and Real-Time Motion Monitoring with Threshold Gating for Frameless Cranial Stereotactic Radiosurgery."

[Med Phys 38.](#)

Li, G., et al. (2013).

"Migration from full-head mask to "open-face" mask for immobilization of patients with head and neck cancer."

[J Appl Clin Med Phys 14\(5\): 243-254.](#)

Mancosu, P., et al. (2016).

"Accuracy evaluation of the optical surface monitoring system on EDGE linear accelerator in a phantom study."

[Med Dosim 41\(2\): 173-179.](#)

Oliver, J. A., et al. (2017).

"Orthogonal image pairs coupled with OSMS for noncoplanar beam angle, intracranial, single-isocenter, SRS treatments with multiple targets on the Varian Edge radiosurgery system."

[Adv Radiat Oncol 2\(3\): 494-502.](#)

Pan, H., et al. (2012).

"Frameless, real-time, surface imaging-guided radiosurgery: clinical outcomes for brain metastases."

[Neurosurgery 71\(4\): 844-851.](#)

Paravati, A. J., et al. (2014).

"Initial clinical experience with surface image guided (SIG) radiosurgery for trigeminal neuralgia."

[Translational Cancer Research 3\(4\): 333-337.](#)

Peng, J. L., et al. (2010).

"Characterization of a real-time surface image-guided stereotactic positioning system."

[Med Phys 37\(10\): 5421-5433.](#)

Pham, N. L., et al. (2014).

"Frameless, real-time, surface imaging-guided radiosurgery: update on clinical outcomes for brain metastases."

[Translational Cancer Research 3\(4\): 351-357.](#)

Sarkar, V., et al. (2018).

"An evaluation of the consistency of shifts reported by three different systems for non-coplanar treatments."

[Journal of radiosurgery and SBRT 5\(4\): 323-330.](#)

Wiant, D., et al. (2018).

"Direct comparison between surface imaging and orthogonal radiographic imaging for SRS localization in phantom."

[Journal of Applied Clinical Medical Physics 0\(0\).](#)

Wiant, D., et al. (2016).

"A prospective evaluation of open face masks for head and neck radiation therapy."

[Pract Radiat Oncol.](#)

Wiersma, R. D., et al. (2013).

"Spatial and temporal performance of 3D optical surface imaging for real-time head position tracking."

[Med Phys 40\(11\): 111712.](#)

Other

Bert, C., et al. (2005).

"A phantom evaluation of a stereovision surface imaging system for radiotherapy patient setup."

[Med Phys 32\(9\): 2753-2762.](#)

Hoisak, J. D. P., et al. (2018).

"The Role of Optical Surface Imaging Systems in Radiation Therapy."

[Semin Radiat Oncol 28\(3\): 185-193.](#)

Li, G., et al. (2016).

"Characterization of optical-surface-imaging-based spirometry for respiratory surrogating in radiotherapy."

[Med Phys 43\(5\): 1348-1360.](#)

O'Connor, M., et al. (2014).

"A Review of the Magnitude of Patient Imaging Shifts in Relation to Departmental Policy Changes."

[Med Phys 41\(158\).](#)

Paxton, A. B., et al. (2017).

"Evaluation of a surface imaging system's isocenter calibration methods."

[J Appl Clin Med Phys 18\(2\): 85-91.](#)

Smith, T., et al. (2016).

"Characterization of a High-Definition Optical Patient Surface Tracking System Across Five Installations."

[Med Phys 43.](#)

Wen, N., et al. (2015).

"Characteristics of a novel treatment system for linear accelerator-based stereotactic radiosurgery."

[J Appl Clin Med Phys 16\(4\): 125-148.](#)

Wen, N., et al. (2016).

"Technical Note: Evaluation of the systematic accuracy of a frameless, multiple image modality guided, linear accelerator based stereotactic radiosurgery system."

[Med Phys 43\(5\): 2527.](#)

Brady, J. L., et al. (2016).

"Analysis of Factors Affecting Benefit from Deep Inspiration Breath Hold Technique in Mediastinal Radiation Therapy for Lymphoma."

[International Journal of Radiation Oncology • Biology • Physics 96\(2\): E491.](#)

Brady, J. L., et al. (2016).

"Deep inspiration breath hold with 'AlignRT' in 3D conformal mediastinal radiotherapy for lymphoma."

[Radiotherapy and Oncology 119: S813-S814.](#)

Gopan, O., et al. (2012).

"Evaluation of the accuracy of a 3D surface imaging system for patient setup in head and neck cancer radiotherapy."

[Int J Radiat Oncol Biol Phys 84\(2\): 547-552.](#)

Zhao B, et al. (2018).

Minimal mask immobilization with optical surface guidance for head and neck radiotherapy.

[J Appl Clin Med Phys 2018;19 \(1\):17-24.](#)